


File D:\DATA\A02\MONITOR\CT -A-199-06799-LCMSA052.D Tgt Mass (CHM):
Injection Date : 23-Dec-19, 09:13:07 Seq. Line : 0
Sample Name : CT -A-199 Lot 09 Location : P1-C-08
Acq. Operator : admin Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Methods\1-HPLC.M
Analysis Method : D:\METHODS\1-HPLC.M
Sample Info : Walkup method: '1-HPLC.M' Target:
Method Info : Mobile Phase: A:Water(10mM NH4HCO3) B:ACN
Gradient: 10% increase to 95%B within 8min,95%B for7 min
Flow Rate: 1.0 ml/min
Column:Xbridge C18,3.5um,4.6*150mm
Column Temperature:40 C
Detection:UV(214,4nm)




DAD1 B, Sig=254.4 Ref=off

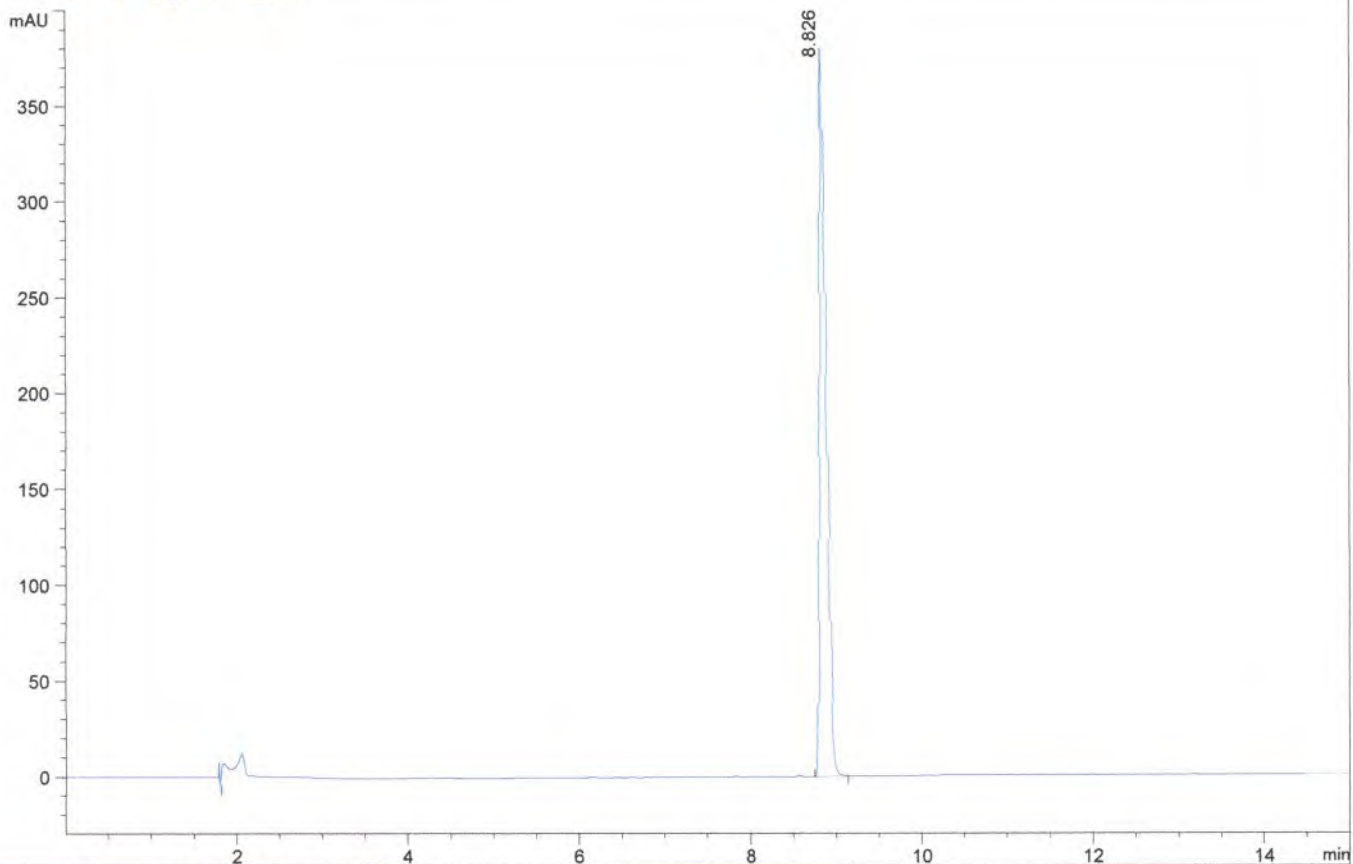

Integration Results for DAD1 B, Sig=254.4 Ref=off

RetTim	Width	Area	Height	Area%
8.83	0.08	2146.23	380.71	100.00

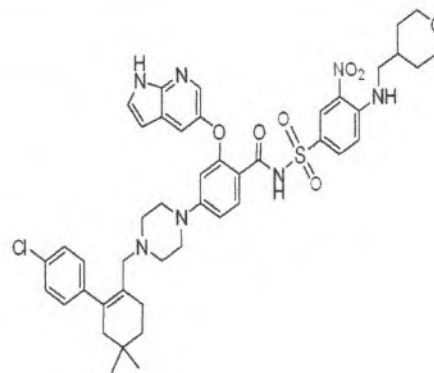

Ret. Time: 8.89

<<<< POSITIVE SPECTRA >>>>

