

File D:\DATA\A02\RS-AC220-05795-HPLCA004.D

Injection Date : 08-Mar-16, 08:55:52

Sample Name : AC220 Lot 04

Acq. Operator : HPLCA004

Spec. Reported : MS Integration

Acq. Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M

Analysis Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M

Sample Info : Easy-Access Method: '2-HPLC-15min'

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 0min 5%B, 3min 5%B, 10min 95%B, 15min 95%B

Flow Rate: 1.2 ml/min

Column: Eclipse XDB-C18, 4.6*150mm, 5um

Oven Temperature: 40 C

Tgt Mass (EZ) :


Location : P1-A-03

Inj : 0

Inj Volume : 1 ul



DAD1 A, Sig=214,4 Ref=off

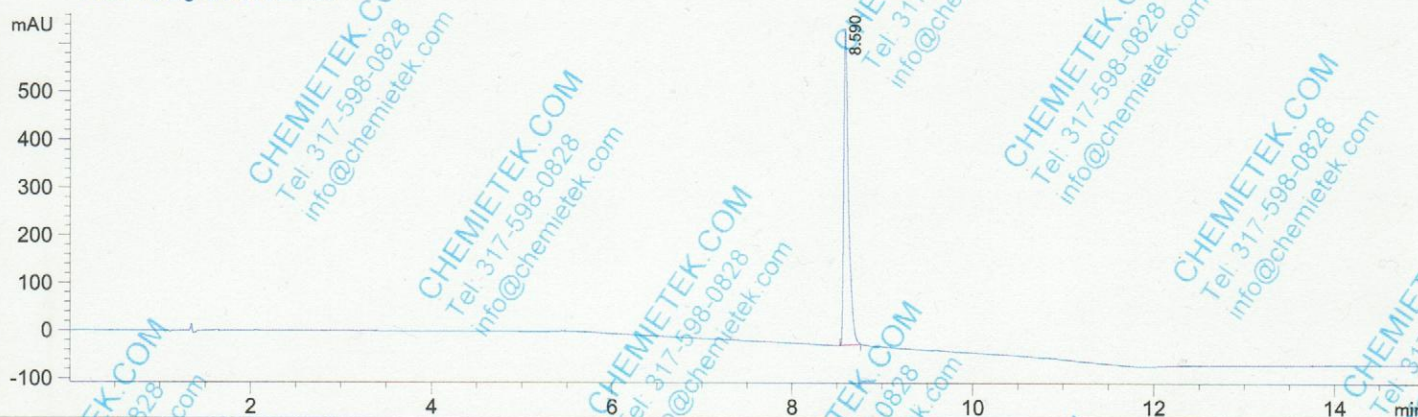

DAD1 B, Sig=254,4 Ref=off



Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
8.59	0.05	2443.11	658.60	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
8.59	0.05	1315.19	353.30	100.00

