

CHEMIETEK HPLC-MS Report

File D:\DATA\A02\MONITOR\SV1-5-1-00870-LCMSA026.D

Injection Date : 26 Oct 12 3:53 pm +0800

Tgt Mass(EZX) : 257.00

Sample Name : AS605240-01

Location : P1-E-06

Acq. Operator : A02-Monitor

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 2 ul

Acq. Method : C:\CHEM32\1\METHODS\1-POS-3MIN.M

Analysis Method : D:\DATA\T67\MONITOR\SP-0009897-085-00712-LCMSA026.D\DA.M

Sample Info : 257.00


Method Info : Mobile Phase : A: water (10mM NH₄HCO₃) B: Acetonitrile

Gradient : 5%B for 0.2min, increase to 95%B within 1.5min,
95%B for 1.5min, back to 5%B within 0.01min.

Flow Rate : 1.8mL/min

Column : XBridge C18 , 4.6*50mm, 3.5um

Oven Temperature : 50 C

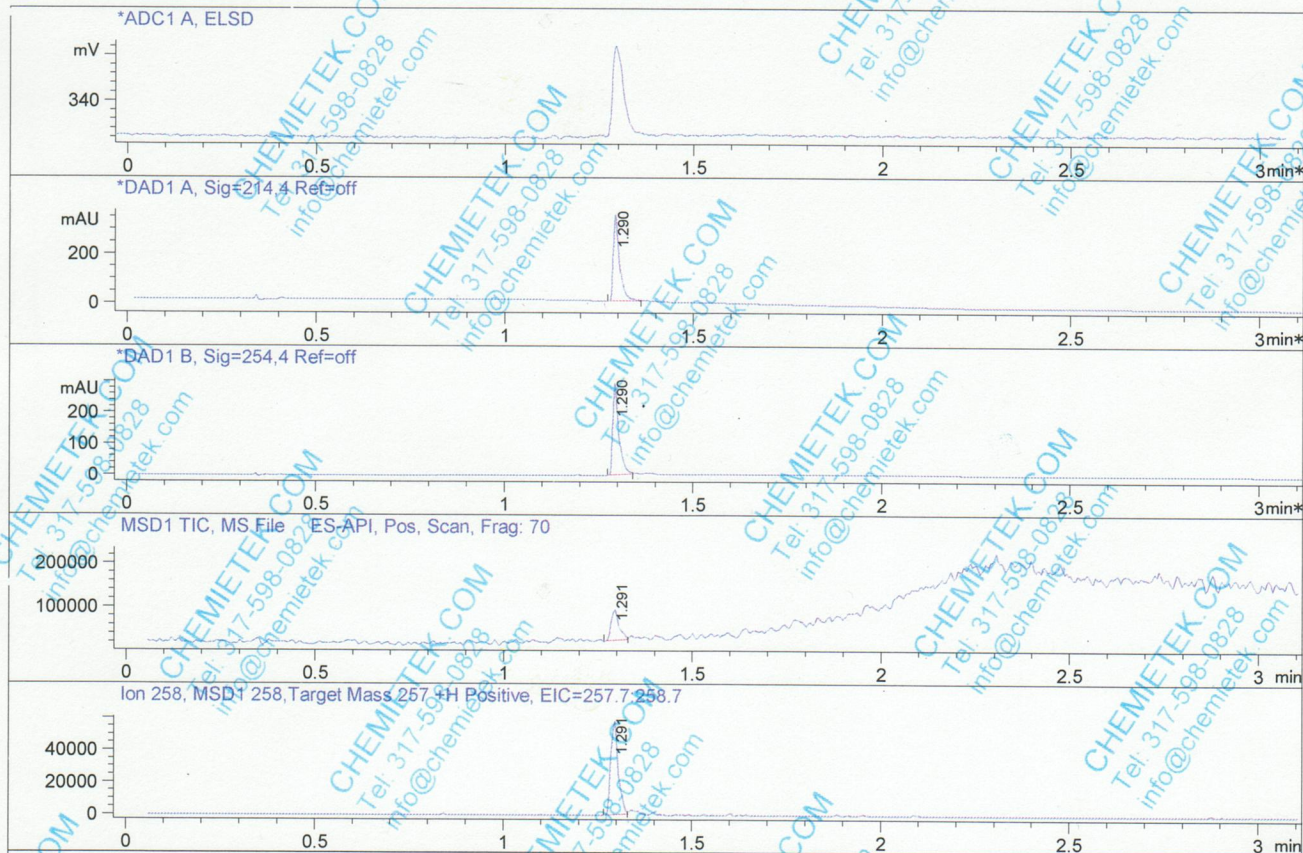

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
--------	-------	------	--------	-------

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.29	0.02	405.47	345.63	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.29	0.02	327.42	290.78	100.00

LC/MS Report

Ret. Time: 1.29

<<<< POSITIVE SPECTRA >>>>

