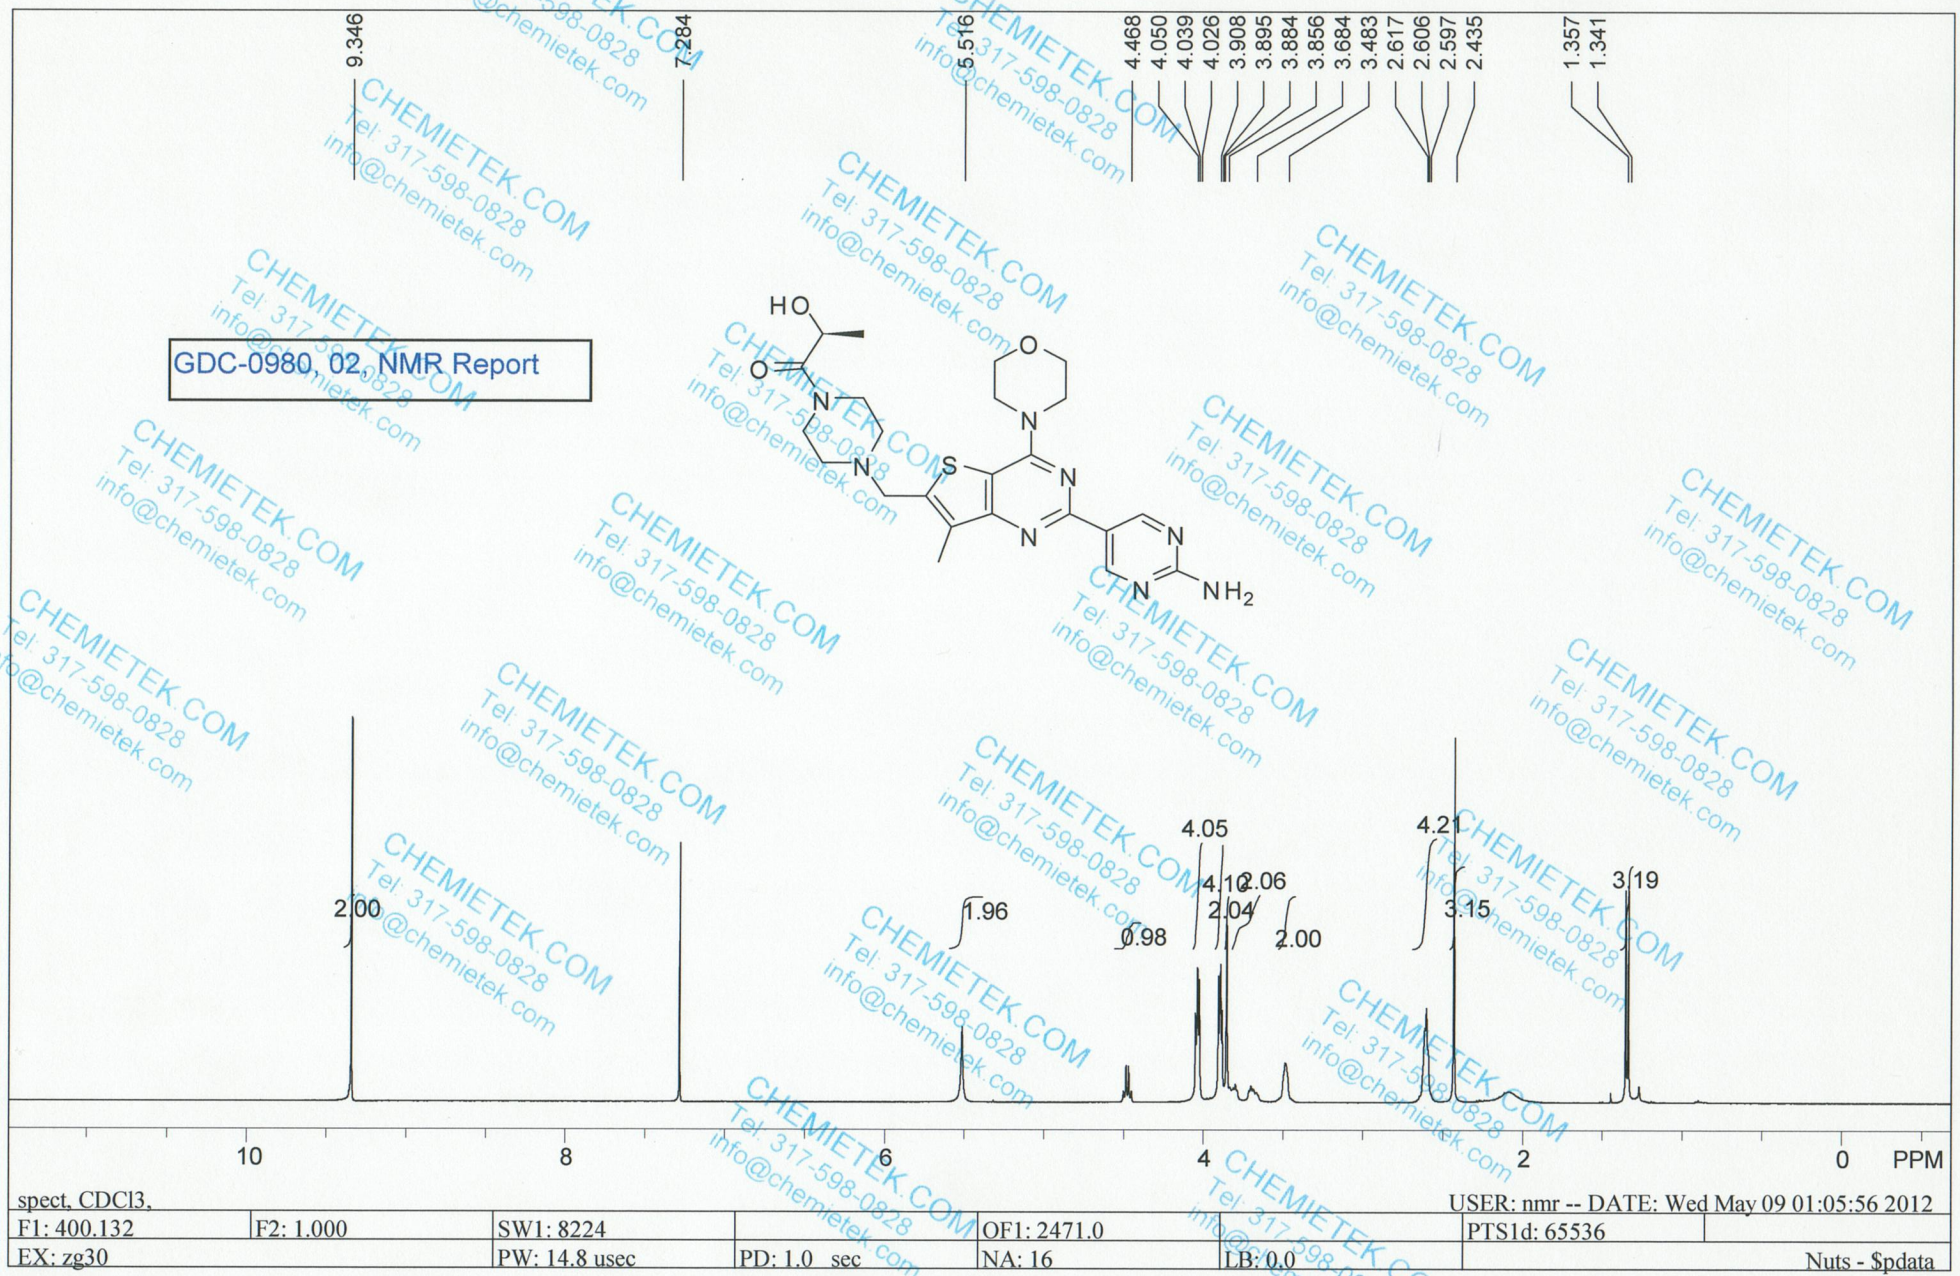

PDF created with pdfFactory Pro trial version www.pdffactory.com

Injection Date Time Stamp	12-05-16 8:40:26 PM
Injection Volume	5
Co-Solvent	MEOH(0.1%DEA)
Column	AS-H (4.6*250mm,5um)
Sample	GDC-0980-02
Sample Well	P1: 1D
Column Temperature	39.9
CO2 Flow Rate	2.1
Co-Solvent Flow Rate	0.9
Co-Solvent %	30
Back Pressure	151
Total Flow	3
PDA Start Wavelength	214
PDA Stop Wavelength	359

Injection Info

Number	RT (min)	Area	Area %	Theoretical Plate
1	4.39	14002.8227	100	2913.4213

Peak Info

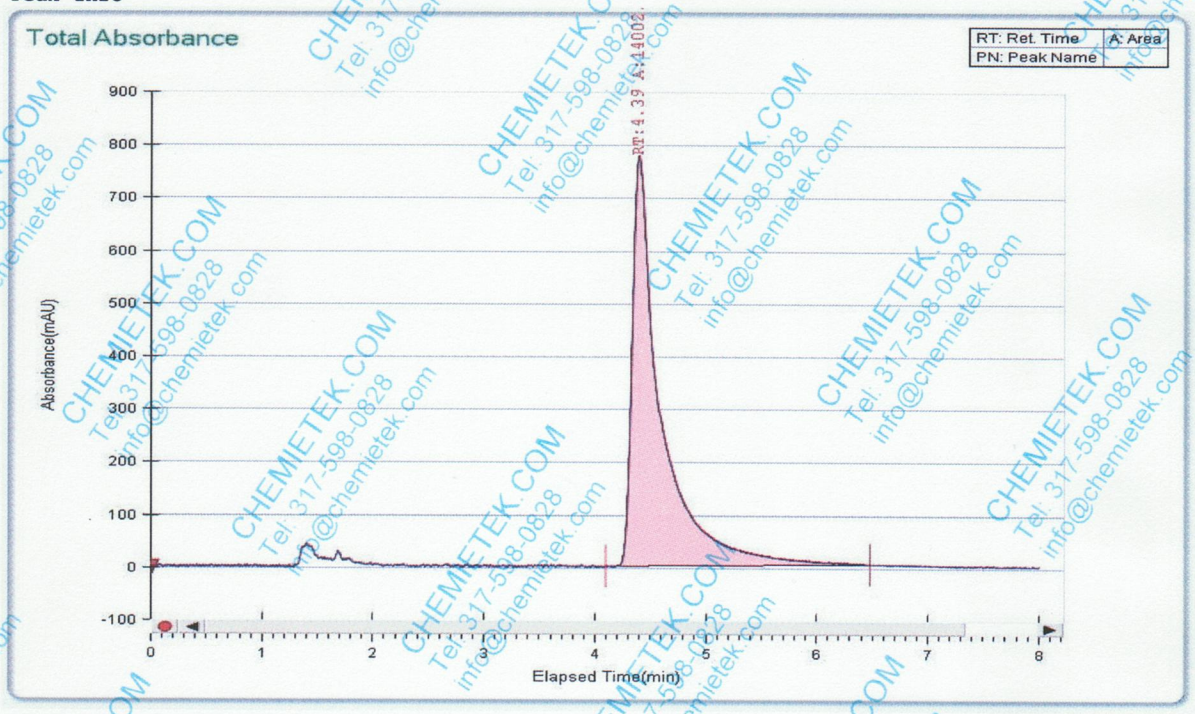

PDASingleSpectrumGraph

PDASingleSpectrumPlot.png

CHEMIETEK.COM Tel: 317-598-0828 info@chemietek.com