

File D:\DATA\A02\MONITOR\GSK-M-A-24061-LCMSA016.D

Injection Date : 11 Mar 20 5:12 pm +0800

Tgt Mass (EZX) :

Sample Name : I-BET-151 05

Location : P2-F-02

Acq. Operator : A02-Monitor

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 1.5 ul

Acq. Method : D:\METHODS\1-POS-15MIN.M

Analysis Method : D:\METHODS\1-POS-15MIN.M

Sample Info : Easy-Access Method: '1-POS-15MIN.M'

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 5%B increase to 95%B within 8.0 min, 95%B for 7.0 min.

Flow Rate: 1.0ml/min


Column: Sunfire C18, 4.6*150mm, 3.5um

Column Temperature: 40 C


Detection: UV(214,4nm) and MS(ESI, Pos mode, 110 to 1500 amu)




*ADC1 A, ELSD

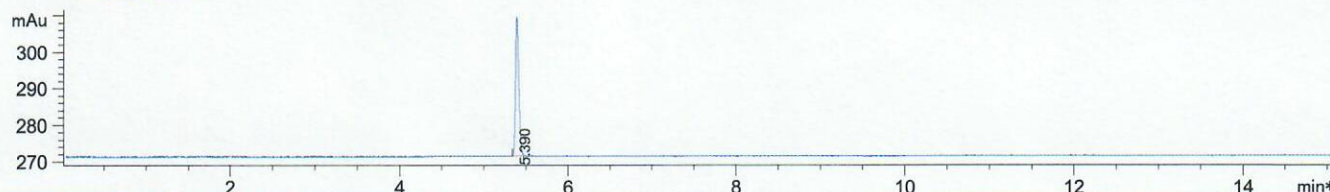


*DAD1 A, Sig=214,4 Ref=off

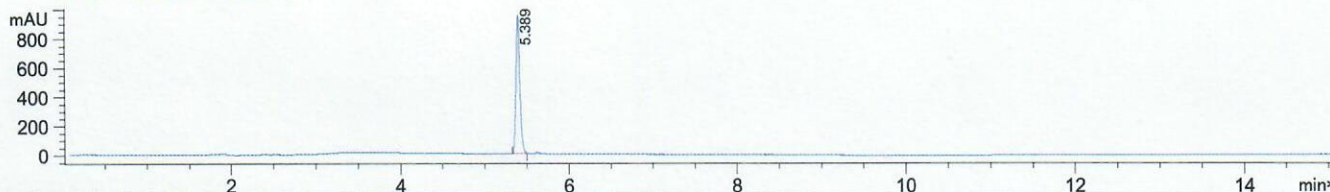

*DAD1 B, Sig=254,4 Ref=off

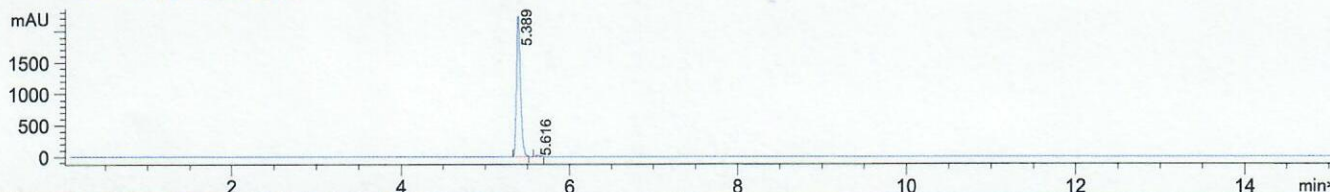

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

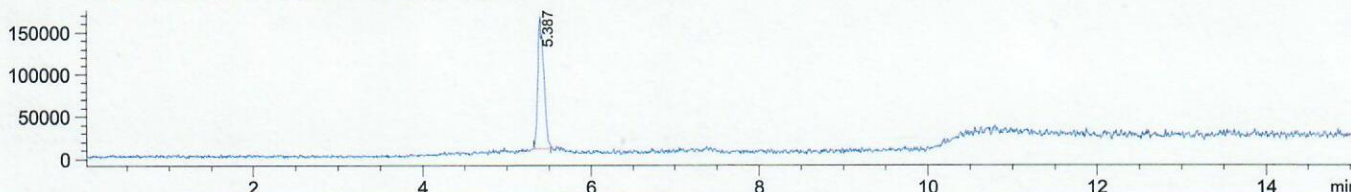

Integration Results for ADC1 A, ELSD


RetTim	Width	Area	Height	Area%
5.39	0.04	104.88	38.40	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
5.39	0.05	3001.99	950.12	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.39	0.05	7294.73	2246.48	99.19
5.62	0.04	59.87	19.70	0.81

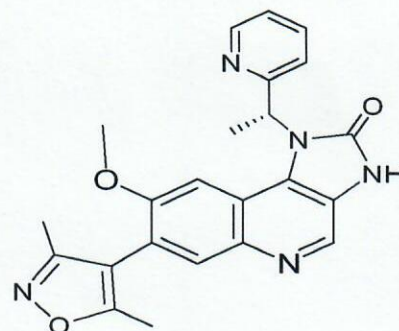

Ret. Time: 5.39

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

